


PROBE SELECTION GUIDE

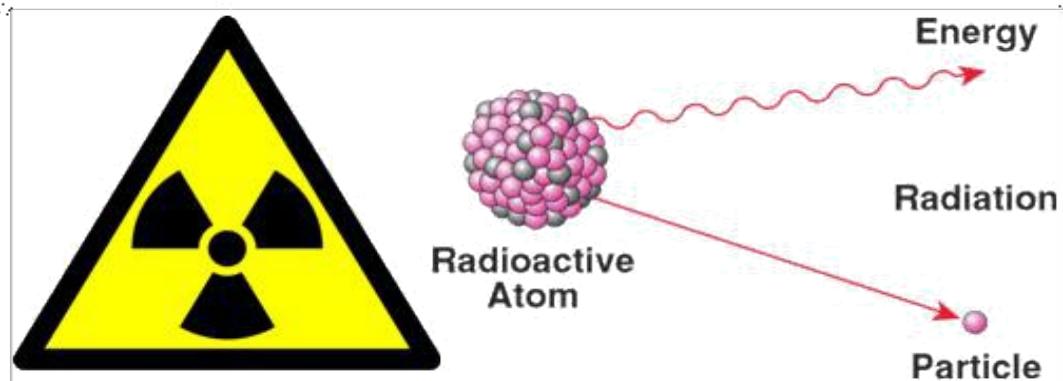

by Massimiliano De Luigi - iz4kjs@tiscali.it AND SalvatoreGiarratana-labx@yahoo.it

last update 10/02/2020

DOSING QUANTITIES		
SI International System	abbreviation	Used to measure
Gray	Gy	- absorbed dose (equivalent to rad) - = 1Gy! joule per kilogram of matter - 1 Gy = 100 rad
Sievert	Sv	- equivalent dose (equivalent to rem) - 1 Sv = Gy x Q - 1 Sv = 100 rem
Becquerel	Bq	- radioactivity (equivalent to Ci) - 1 Bq = 1 disintegration / second - $3,7 \times 10^{10}$ Bq = 37 billion Bq = 1 Ci

Unita USA	abbreviation	Used to measure
Roentgen	R	- exposure (obsolete) - measures the amount of ionization in air - $1 R = 2,58 \times 10^{-4}$ coulomb x kg of dry air
Rad (Radiation absorbed dose)	rad	- absorbed dose of energy from any material - $1 \text{ rad} = 100 \text{ ergs per gram of matter}$
Rem (Roentgen equivalent man)	rem	- dose equivalent to biological damage in human tissue - rem = rad x Q (quality factor) - Q = 1 X-ray, up to 20 neutrons or alpha
Curie	there	- radioactivity - $1 \text{ Bq} = 1 \text{ disintegration / second}$ - $1 \text{ There amount of matter that emits } 3,7 \times 10^{10} \text{ dis / sec}$

MITIGATION THICKNESS TO A TENTH TO DIFFERENT nuclides / MATERIALS						
material	lead	Glass at Lead	Iron	Concrete Barium	concrete	bricks
density g / cm ³						
Co 60	11,34 4 cm	Variable, P 47 / cm P	7.8 7 cm	3.2 16 cm	2.3 22 cm	1.4 36 cm
Cs 137	2,1 cm	32 / cm P	5,5 cm	12 cm	17 cm	28 cm
ir 192	1.7 cm	25 / cm P	4.5 cm	10 cm	14 cm	23 cm


"Inverse square law of the distance"

example: measure 10 millirem / hour up to 10 cm from the source, the measurement at 20 cm distance will be 2.5 millirem / hour by calculating the dose to 20 cm = $10 \text{ mrem / hr} \times (10 \text{ cm} / 20 \text{ cm})^2 = 2.5 \text{ mrem / hr}$
therefore small changes in distance from the source correspond in large exposure intensity changes

A small example to understand the difference between the various units of measurement:


Imagine you're in the rain, the amount of rain fall is measured in Becquerel, the amount of rain hitting is measured in Gray, as it is wet on the body is measured in Sievert.

See website <http://www.darvill.clara.net/nucrad/units.htm>

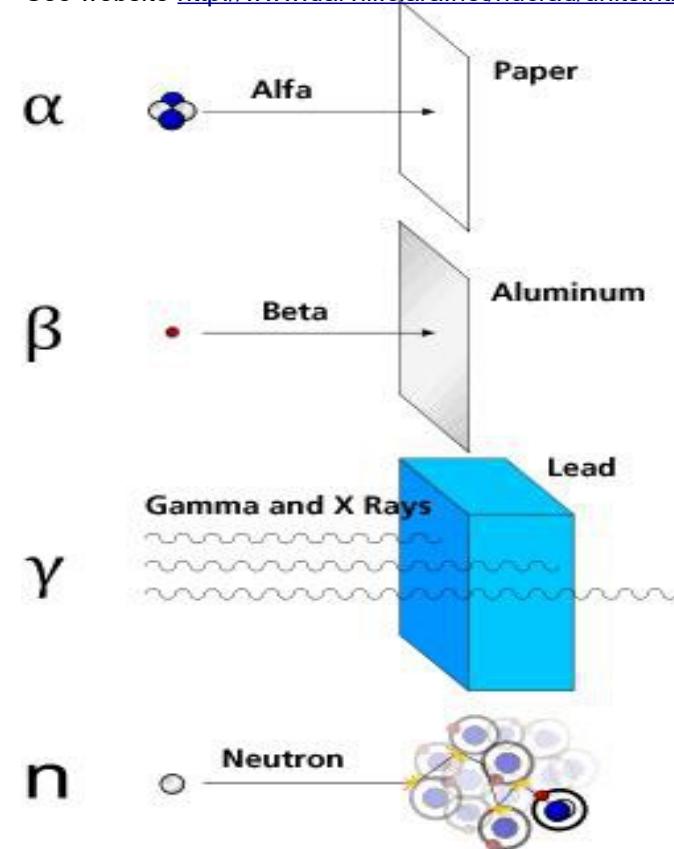

TYPES OF RADIATION			
Guy	Alpha	Beta	Range
symbol	α	β	γ
Atomic mass	4	1/1840	0
charge	+2	-1 or +1	0
speed	low	high	vel. Light
ioniz capacity.	high	average	0
range in the air	3 cm	3 m	high
range in tissue	0.04 mm	5 mm	high
stopped by	sheet of paper	mm aluminum	cm lead

EFFECT OF VARIOUS TYPES OF RADIATION		
radiation	process	effect
Alpha	Inelastic collisions with electrons bound	Excitation and ionization
Beta	Coll. Inel. Electr. atomic	Excitation and ionization
	Bremsstrahlung in the field nuclear	emissions Bremsstrahlung
X-rays and Range	Photoelectric Effect	Photon tot. Absorbed
	Compton Effect	Photon parz. Absorbed
	Production of Couples	

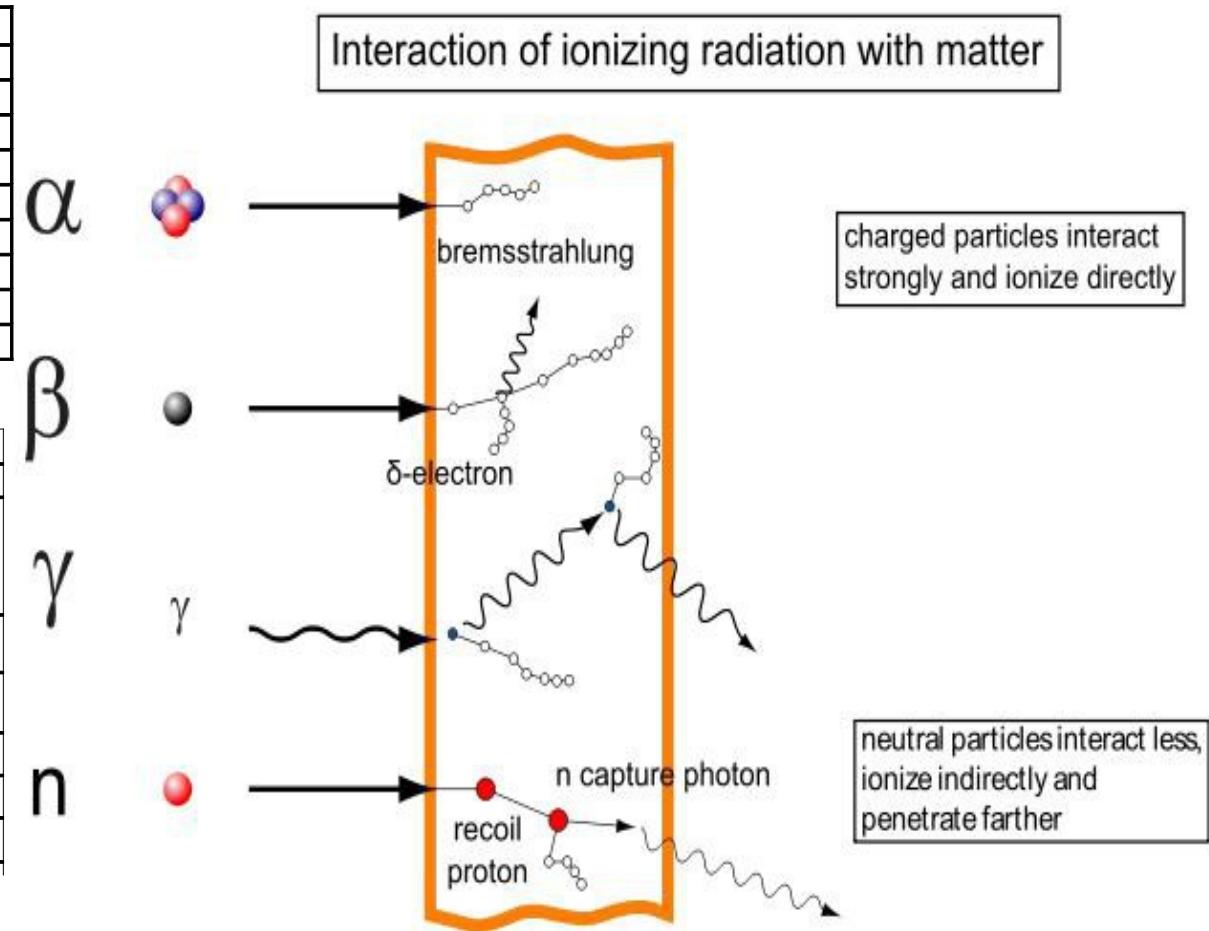

radioisotope	Half-Life	significant Radiations	Comments
Sodium-22	2.6 yr	0:54 MeV positron; 00:51 and 1.27 MeV gammas	high beta and gamma dose rates
Iron-55	2.7 yr	Various low energy x-rays and Auger electrons (<6 keV)	does not present a significant external hazard
Cobalt-57	271.8 days	Gammas (<than 00:13 MeV)	
Cobalt-60	5.3 yr	0:31 MeV beta; 1:17 and 1:33 MeV gammas	high beta and gamma dose rates
Nickel-63	100 yr	0.066 MeV beta	does not present a significant external hazard
Strontium-90	29.1 yr	0:54 MeV beta from Sr-90; 2:26 MeV beta from Y-90	decays to short-lived Y-90; very high beta dose rates
Cesium-137	30.1 yr	0:51 MeV beta; 0661 range from Ba-133m	decays to short-lived Ba-133m
Polonium-210	138.4 days	5.3 MeV alpha	does not present a significant external hazard
Radium-226	1600 yr	4.8 MeV alpha; various alphas, betas and gammas from decay	decays to Rn-222, with a long decay Following chain
Americium-241	432.7 yr	5.6 MeV alpha; various alphas, betas and gammas from decay	decays to Np-237 long-lived, decaying in turn to Pa-233 and U-233. Alpha emissions are the greatest concern.

radioisotope	Beta dose rate at 30 cm from source * (Millirem / hr for millicuries)	gamma dose rate at 30 cm from source (Millirem / hr for millicuries)
Sodium-22	370	13.3
Cobalt-57	0	0.94
Cobalt-60	48	14.4
Strontium-90	740	0
Cesium-137	777	4.1
Americium-241	0	0.56

* Keep in mind That the annual skin dose limit is 50,000 mrem. Working for extended periods in close proximity with certain Radioisotopes can lead to large doses.

see website <http://www.ehs.washington.edu/rsotrain/sealedsources/worksafely.shtm>

Nuclear Radiation Detectors Scheme of detection of energetic charged particles Of SS Kapoor, V. Ramamurthy

Detection method	Detector type	Detection medium
Detection of Free Charge Carriers	Ionization Chambers	Gases Semi-conductors You Ge Condensed forms of noble elements
	Proportional counters	Gases Liquids of noble elements
	Geiger-Muller counters and Avalanche counter	Gases
Light Sensing	scintillation Detectors	inorganic Crystals Organic Liquids and plastic Noble elements
	Cerenkov Detectors	Gases, liquids and solids Trasparent
Detection of free Charge Carriers + Light sensing	Hybrid Detectors	Gases, liquids and of noble elements (Argon, Xenon)
Track Visualization	Track Etch Detector	Minerals Glass Plastic

List (not exhaustive) of the materials used in scintillation detection systems

Bi4Ge3O12	Bismuth germanate
CaF ₂	Calcium Fluoride
CaF ₂ (Eu)	Europium doped Calcium Fluoride
CdWO ₄	Cadmium Tungstate
CsI	Cesium Iodide
CsI (Na)	Sodium doped Cesium Iodide
CsI (Tl)	Thallium doped Cesium Iodide
KBr	Potassium Bromide
KCl	Potassium Chloride
KI	Potassium Iodide
LiF	Lithium Fluoride
NaCl	Sodium Chloride
Nal	Sodium Iodide
Nal (Tl)	Thallium doped Sodium Iodide
rbcL	Rubidium Chloride
ZnWO ₄	Zinc Tungstate
BaF ₂	Barium Fluoride
brilliance 350	Cerium doped Lanthanum Chloride (LaCl ₃)
Lithium Glass Scintillators	Cerium activated lithium silicate glass scintillators
YAG (Ce)	Cerium doped Yttrium Aluminum Garnet
BGO	Bismuth germanate
brilliance 380	Cerium doped Lanthanum Bromide (LaBr ₃)
CsI (pure)	Undoped Cesium Iodide
fibers	Plastic Scintillating, Wavelength-shifting, Light Transmitting, and Fluorescent Fibers
Nal (Tl)	Thallium doped Sodium Iodide Nal (Tl) and Polyscin® Nal (Tl) Scintillation Material
PRELUDE 420	Cerium doped lutetium based (LYSO)

List (not exhaustive) of the most common gas used in Geiger Muller detectors

Gas	symbol	W (eV)	And drift speed	Electric field
	chemist		cm / mS	V * 1 * cm-torr-1
Neon	Neither	36.2		
Argon	Ar	26.4	0.4	0.8
Krypton	Kr	24		
Xenon	Xe	21.7		
Methane	CH ₄	29.1	10	1
ethylene	C ₂ H ₄	28	0.5	1
Iso-butane	IC ₄ H ₁₀	26.3	2.5	1
Isobutylene	IC ₄ H ₈	26.7		
heptane	C ₇ H ₁₆		1.4	1
Carbon Dioxide	CO ₂	20	9	8
Ar + 10% CH ₄			5.5	0.2




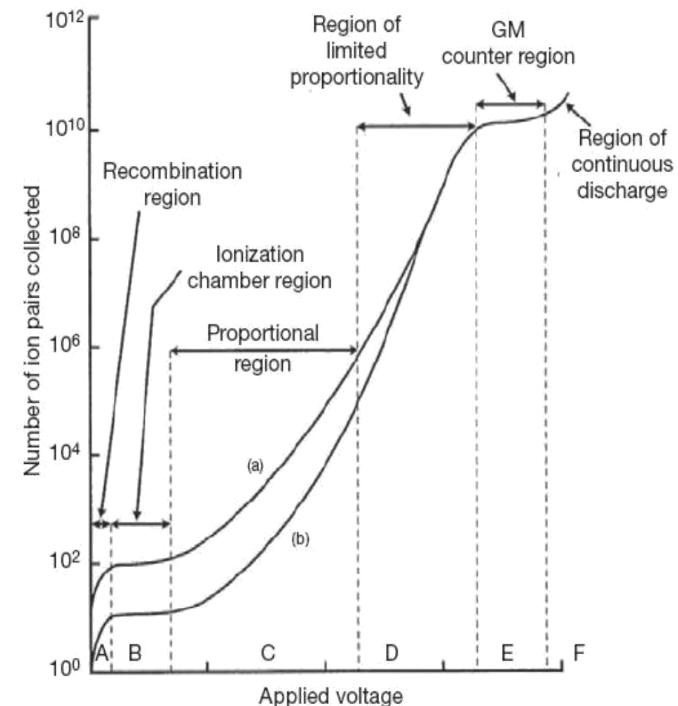


FIG. 4.1. Various regions of operation of a gas filled detector. Region A represents the recombination region, region B the ionization region, region C the proportionality region, region D the region of limited proportionality and region E the GM region. Curve (a) is for 1 MeV β particles, curve (b) for 100 keV β particles.

typical connection diagrams of geiger tubes

see website <http://www.ludlums.com/> > Support> connector type

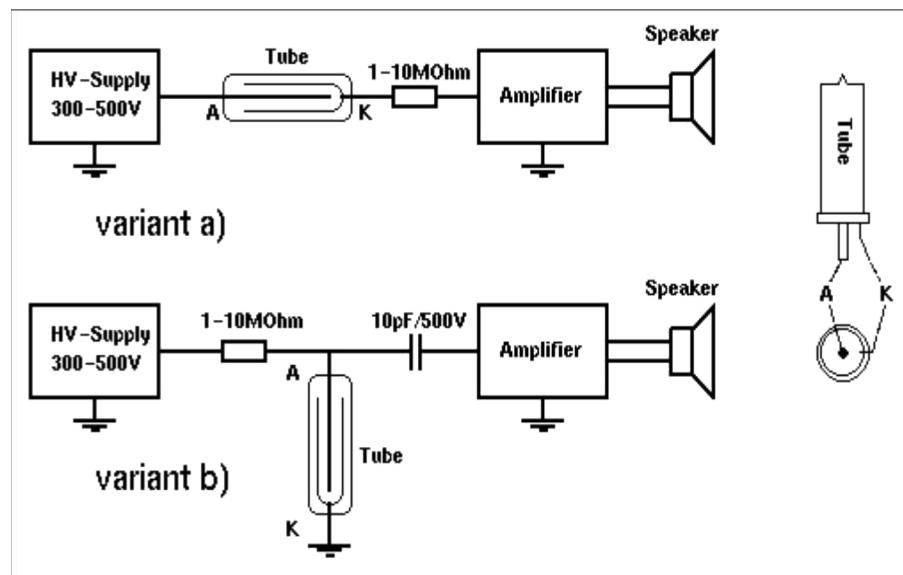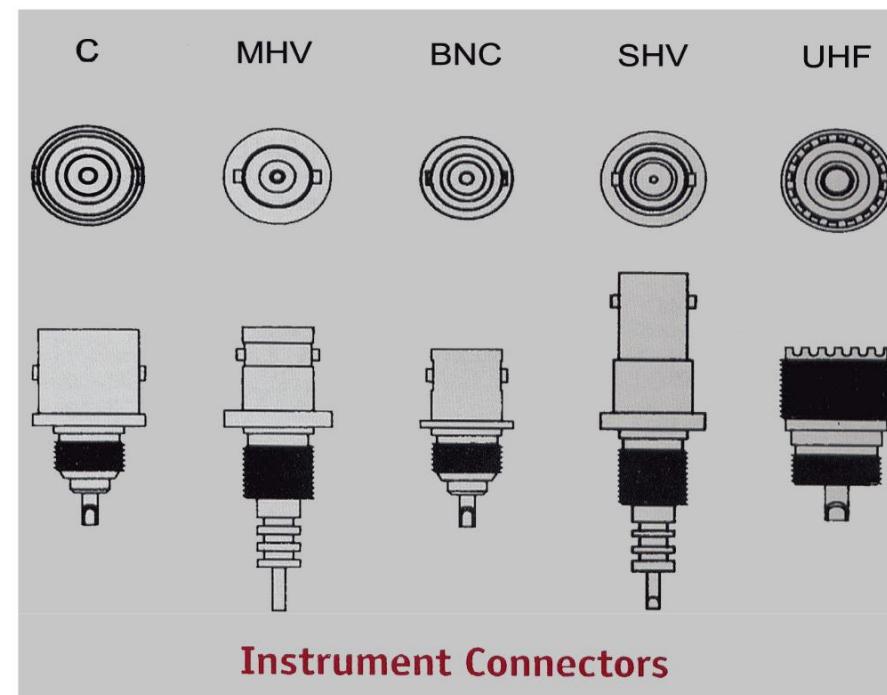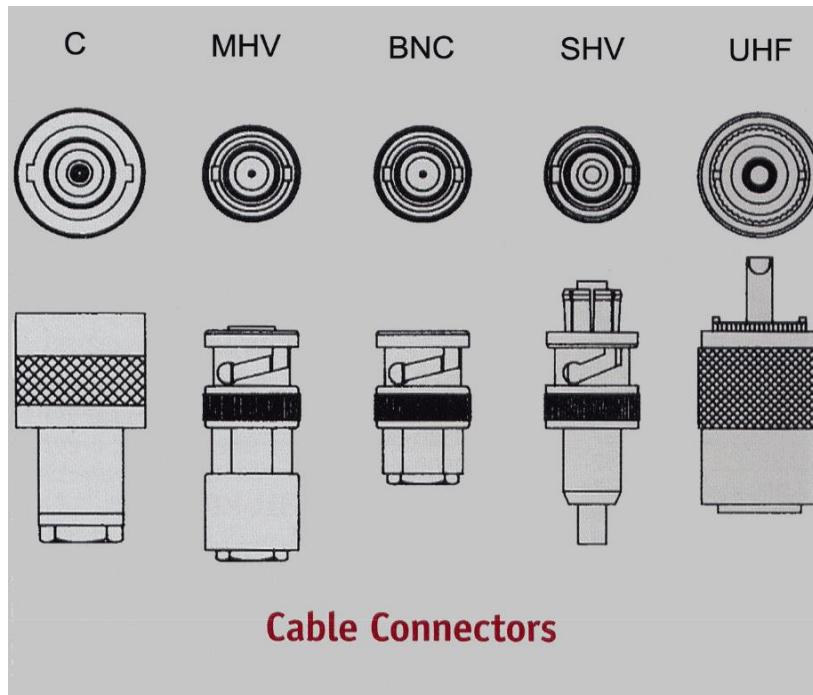

LEGEND

(CPM / mR / hr * 60min / h)	DT - dead time, statistical correction, probe insensitivity time, important <u>only for high values of pulses</u> (available from the manufacturer)
CC = _____ 0.001 R / mR as an example a probe Pancake Ludlum44 / 9 with 3300CPM / mR / hr sensitivity CC = $(3300 \times 60) / 0.001 = 19.8 \times 10^7$ cont / R on the tools marked with: cc = 19.8 + 07	

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	γ Co60	PROBE AREA cm ²
producer	template	type probe	(Volt)	alpha a	beta	range				surface sensitive area	

the probe responds in a different manner according to the voltage of power and as a function of the isotopes present.
in figure 4.1 are summarized 6 operating regions

A- The A PROBE OF EFFICIENCY WITH SOURCES AND ALPHA MAX 15% EFFICIENCY AND BETA B- 'DISCOVERABLE WITH THE FOLLOWING FORMULA:

(Measured CPM - CPM background)
 $Ef * 100\% = \frac{\text{Measured CPM} - \text{CPM background}}{\text{DPM sample source}}$

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr ^{137}Cs	Co60 γ	PROBE AREA cm ²
Amperex	6980	HOT DOG	900		X	X		100		720		
Amperex	100NB	END WINDOW	900		X	X		100				
Amperex	120NB	END WINDOW	900	X	X	X		300				
Amperex	1B85	HOT DOG										
Amperex	200NB	END WINDOW	900	X	X	X		200				
Amperex	85NB	HOT DOG	900		X	X		100		720		
ANTON	114	HOT DOG	900		X	X		100		720		
ANTON	6993	HOT DOG	900		X	X	43.2 + 06	100		720	12.0%	
BICRON	PGM	PANCAKE	900	X	X	X				900		

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
CANBERRA	2000	PANCAKE	900	X	X	X		50		3500		
CANBERRA	2001	PANCAKE	900	X	X	X		50				
CANBERRA	2006	PANCAKE	900	X	X	X		70		3500		
CANBERRA	2011	PANCAKE	900	X	X	X		90		1500		
CANBERRA	2100	END WINDOW	750	X	X	X		50		50		
CANBERRA	2106	END WINDOW	900	X	X	X		70		500		
CANBERRA	2111	END WINDOW	500	X	X	X		90		1200		
CANBERRA	2112	END WINDOW	500	X	X	X		90		1200		
CANBERRA	2121	END WINDOW	575	X	X	X		100		1700		
CANBERRA	2123	END WINDOW	900									
CANBERRA	2126	END WINDOW	900	X	X	X		150		2700		
CANBERRA	2131	END WINDOW	900	X	X	X		200		1650		
CANBERRA	2135	END WINDOW										
CANBERRA	2200	THIN WALL	900		X	X		100		5275		
CANBERRA	2202	THIN WALL	900		X	X		75		2900		
CANBERRA	2206	THIN WALL	900		X	X		90		635		
CANBERRA	2211	THIN WALL	900		X	X		150		1550		
CANBERRA	2216	THIN WALL	900		X	X		150		4800		
CANBERRA	2300	THIN WALL	900			X		20		175		
CANBERRA	2305	THIN WALL	500			X		90		1200		
CANBERRA	2306	THIN WALL	900			X		100		950		
CANBERRA	2311	THIN WALL	900			X		100		1880		
CANBERRA	2314	THIN WALL	900			X		100		3050		
CANBERRA	2316	THIN WALL	900			X		100		3950		
CANBERRA	2350	THIN WALL	900			X		120		8150		
CANBERRA	2406	MINIATURE	550			X		11		19		
CANBERRA	2411	MINIATURE	575			X		15		54		
CANBERRA	2416	MINIATURE	575			X		28		420		
CANBERRA	2420	MINIATURE	500			X		10		4		
CANBERRA	2422	MINIATURE	460			X		10		1		
CANBERRA	2423	MINIATURE	550			X		10		1		
CANBERRA	JAN5979	MINIATURE	700	X	X	X		150		2700		
CANBERRA	JAN7616	MINIATURE	760	X	X	X		75		600		
CANBERRA	P2121S	END WINDOW	900	X	X	X		100		1700		

see website <http://www.canberra.com/products/438339.asp>

Characteristics	T2411M	T2416A	T2417A	T2420M	T2422	3G70 / EM14752 3G70	4G60M / EM14754 4G60M	4G2500 / EM14749 4G2500	3G6500 / EM14748 3G6500
Sensitivity *** 137Cs cpm at 1 mR / h *	84	420	450	4:02:00	1:06:00	4:02:00	4:02:00	150	270
Window Area Density (Mg / cm ²)	N / A	N / A	N / A	N / A	N / A	N / A	N / A	N / A	N / A
Window Effective Diameter (Mm, in.)	N / A	N / A	N / A	N / A	N / A	N / A	N / A	N / A	N / A
Recommended Operating Voltage (HV +)	575	575	575	500	460	460	500	550	460
Plateau Length Volts min.	500-650	500-650	500-650	450-550	450-550	420-500	450-550	500-600	420-500
Plateau Slope (% 100 V max.)	15	8	8	35	40 max.	30	30	25	25
Dead Time (s max.)	15	45	45	20	10	25	25	35	50
Background (cpm)									
Shielding 2 "Pb + 1/8" At	2 max.	12 max.	5 max.	6 typ.	0.6 typ.	0.6 max.	0.6 max.	6 max.	10 max.
Resistor Ra (MΩ)	2.2 M	4.7 M	4.7 M	4.7 M	4.7 M	4.7 M	4.7 M	4.7 M	4.7 M
Operating Temp. (° C)	-40 to +75	-40 to +75	-40 to +75	-51 to +71	-20 to +60	-20 to +60	-20 to +60	-20 to +60	-20 to +60
Cathode Material	Cr / Fe	Cr / Fe	Cr / Fe	Cr / Fe	Cr / Fe	Cr / Fe	Cr / Fe	Cr / Fe	Cr / Fe
Cathode Wall	80-100 mg / cm ²	64-80 mg / cm ²	64-80 mg / cm ²	360-400 mg / cm ²	360-400 mg / cm ²	360 mg / cm ²	360 mg / cm ²	260 mg / cm ²	280 mg / cm ²
Max. Overall Length including Pins (mm, in.)	37-1:46	51- 2.0	46 -1.82	20 -0.8	20 -0.8	34- 2.91	20- 2:36	34-2.91	54- 3.7
Max. Overall Diameter (mm, in.)	6.2- 0.244	10- 0.4	9,20- 0:36	7-0,28	7- 0,28	7- 0,28	7- 0,28	7- 0,28	7- 0,28
Window Recess (mm, in.)	N / A	N / A	N / A	N / A	N / A	N / A	N / A	N / A	N / A

* An exposure of 115.07 mR in air equates to 1.0 mGy.

*** At recommended operating voltage.

The T2422 detector is equivalent to the 3G10.

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
CENTRONIC	B12H											
CENTRONIC	B12H / FL		370		X	X				5600		
CENTRONIC	B6H		650		X	X				5600		
CENTRONIC	B6TS		370		X	X				2000		
CENTRONIC	C1300		500		X	X		7				
CENTRONIC	C300		500		X	X		11				
CENTRONIC	C301		500			X		7				
CENTRONIC	M2H											
CENTRONIC	M6H / 100											
CENTRONIC	ZP1200	THIN WALL	500		X	X		90		19		
CENTRONIC	ZP1201		400			X		70				
CENTRONIC	ZP1202		400			X		110				
CENTRONIC	ZP1206		450			X		70				
CENTRONIC	ZP1210		400			X		200				
CENTRONIC	ZP1211 / 02		400			X		200				
CENTRONIC	ZP121221											
CENTRONIC	ZP1220		400			X		210				
CENTRONIC	ZP1220 / 01		400			X		210				
CENTRONIC	ZP1220 / EC		400			X		210				
CENTRONIC	ZP1221		500			X		210				
CENTRONIC	ZP1221 / 01		400			X		210				
CENTRONIC	ZP1221 / 02		400			X		210				
CENTRONIC	ZP1300	THIN WALL	550		X	X		11		54		
CENTRONIC	ZP1301		500			X		13				
CENTRONIC	ZP1302		500			X		13				
CENTRONIC	ZP1304		500			X		13				
CENTRONIC	ZP1310	THIN WALL	575		X	X		15		3950		
CENTRONIC	ZP1313		500			X		15				
CENTRONIC	ZP1314		500			X		15				
CENTRONIC	ZP1320		500		X	X		45				
CENTRONIC	ZP1320	THIN WALL	900					100		4		
CENTRONIC	ZP1321		500			X		55				
CENTRONIC	ZP1324		500			X		55				

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr ^{137}Cs	Co60 γ	PROBE AREA cm ²
CENTRONIC	ZP1352		600		X	X		200				
CENTRONIC	ZP1400	END WINDOW	500		X	X		90		1200		
CENTRONIC	ZP1401	END WINDOW	500		X	X		90		1200		
CENTRONIC	ZP1402		400	X	X	X		110				
CENTRONIC	ZP1405		400	X	X	X		110				
CENTRONIC	ZP1410	END WINDOW	575		X	X		100		1200		
CENTRONIC	ZP1430		450	X	X	X		230				
CENTRONIC	ZP1431		500	X	X	X		230				
CENTRONIC	ZP1441		500	X	X	X		65				
CENTRONIC	ZP1442		500		X	X		65				
CENTRONIC	ZP1450	PANCAKE	900	X	X	X		90		1500		
CENTRONIC	ZP1451		500	X	X	X		60				
CENTRONIC	ZP1452		400		X	X		60				
CENTRONIC	ZP1480		400	x	X	X		120				
CENTRONIC	ZP1481		450	X	X	X		120				
CENTRONIC	ZP1490		500			X		65				

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

see website http://www.centronic.co.uk/standard_products.htm

Type	Sensitivity			Plateau			Counting Rate Acts	Dead Time (MS)	back- Ground Shielded (Counts / min.)	Dose Rate Range (MGy / h)
	Band	Length	Threshold	Length	Slope					
	α	β	γ	(Mm)	(V) max.	(V)	(% / V) max.	(Counts / s) ♦	max.	typical
ZP1200		.	40	400	200	0.04	28	90	10	10-3 - 102
ZP1206		.	14.5	450	100	0.1	11	70	9	1.5 x 10-3 - 2 x 102
ZP1210		.	140	400	100	0.15	110	200	70	3 x 10-4 - 10
ZP1220		.	240	400	100	0.15	180	210	90	2 x 10-4 - 3
ZP1220 / EC *		.	240	400	100	0.15	180	210	90	2 x 10-4 - 3
ZP1220 / 01		.	240	400	100	0.15	180	210	60	2 x 10-4 - 3
With compensating filter										
ZP1221 / 01		.	240	400	100	0.15	180	210	60	2 x 10-4 - 3
ZP1201		.	40	400	200	0.04	20	110	10	10-3 - 40
ZP1221		.	240	400	100	0.15	180	210	90	2 x 10-4 - 3
ZP1301		.	7	500	100	0.3	340 ♦	13	1	10-1 - 1 x 104
ZP1302		.	7	500	100	0.3	340 ♦	13	12-120	10-1 - 1 x 104
ZP1313		.	16	500	150	0.15	1600 ♦	15	2	10-2 - 1 x 103
ZP1321		.	28	500	150	0.08	9	55	12	3 x 10-3 - 102
Ambient dose compensated										
ZP1202		.	40	400	200	0.04	20	110	10	10-3 - 40
ZP1211 / 02		.	140	400	100	0.15	110	200	60	3 x 10-4 - 10
ZP1221 / 02		.	240	400	100	0.15	180	210	60	23 x 10-4 - 3
ZP1304		.	7	500	100	0.3	340 ♦	13	1	10-1 - 1 x 104
ZP1314		.	16	500	150	1.15	1600 ♦	15	2	10-2 - 1 x 103
ZP1324		.	27	500	150	0.08	9	55	12	3 x 10-3 - 102
ZP1300	.	.	7	500	100	0.3	300 ♦	11	1	10-1 - 104
ZP1310	.	.	16	500	150	0.15	1600 ♦	15	2	2 x 10-2 - 4 x 103
ZP1320	.	.	28	500	150	0.08	9	45	12	3 x 10-3 - 2 x 102
ZP1352	.	.	120	400-600	200	0.01	85	200	35	3 x 10-4 - 10
ZP1400	.	.	9c	400	200	0.04	25	90	10	10-3 - 102
ZP1431	.	.	27.8a	450	250	0.04	44	230	25	6 x 10-4 - 6
ZP1442	.	.	19.8c	500	200	0.09	16	65	9	10-3 - 102
ZP1452	.	.	17.8c	500	250	0.07	29	60	25	10-3 - 20
ZP1480	.	.	17d	400	100	0.2	24	120	30	10-3 - 20
ZP1481	.	.	17d	400	100	0.2	24	120	30	10-3 - 20
ZP1401	.	.	9a	400	200	0.04	25	90	10	10-3 - 102
ZP1405	.	.	40	400	100	0.04	20	110	10	10-3 - 102

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

ZP1430	.	.	.	27.8a	450	200	0.04	44	230	25	6 x10-4 - 6
ZP1441	.	.	.	19.8a	500	200	0.09	16	65	9	3 x10-3 - 102
ZP1451	.	.	.	27.8a	500	250	0.07	29	60	14	10-3 - 20
ZP1490	.	.	.	28th	450	250	0.06	29	65	15	10-3 - 20
With compensating filter											
ZP1402	.	.	.	9a	400	200	0.04	20	110	10	10-3 - 102

Type	Sensitivity			Plateau			Counting Rate Acts	Dead Time	back- Ground Shielded	Dose Rate Range
	Band	Length	Threshold	Length	Slope	10-2mGy / h				
	α	β	γ	(Mm)	(V)	(% / V)	(Counts / s) ♦	(M2)	(Counts / min.)	(MGy / h)
C300	.	.	9	500	150	0.02	170◊	7	1	10-1 - 105
C1300	.	.	7	500	100	0.03	360◊	11	1	10-1 - 2 x 104
With compensating filter										
C301	.	.	9	500	150	0.02	140◊	7	1	10-1 - 105

Type	Sensitivity		Operating	Min.	Max.	Active	Life	Sensitivity	Shielded	Background	Liquid Capacity ml	Temp.	Temp.	Coeff. V	Wall / Window	
	Band	Voltage														
	α	β	γ	V	V	mm	counts	expectation	cpm / mR / hr	cpm	ml	Range ° C	° C			mg / cm2
B6H	.	.	.	370	100	0.15	64	1010	2000	15	-	-55 to +60	0.2	25 to 35		
B12H	.	.	.	370	100	0.15	123	1010	5600	30	-	-55 to +60	0.2	25 to 35		
B12N	.	.	.	675	120	0.1	120	1010	5000	30	-	-60 to +70	0.2	25 to 35		
B6T	.	.	.	675	100	0.1	60	1010	-	-	-	-60 to +70	0.1	25 to 35		
With compensating filter																
B6TS	.	.	.	675	100	0.1	60	1010	2700	-	-	-60 to +70	0.1	-	-	
Liquid Sampling																
M6H	Liquid	370	100	0.15	60	1010	-	16	9	-10 to +50	0.2	25 to 35				
M6H / 100		500	200	0.15	60	1010	2880	100	100	-10 to +50	0.2	25 to 35				
M2Na,		510	90	0.15	21	1010	-	20	3.5	-10 to +50	0.2	25 to 35				
M2H,		370	100	0.15	20	1010	-	7	3.5	-55 to +60	0.2	25 to 35				

, Supplied with waterproof rubber jacket

= * = End connector

◊ = Counting rate at 10 mGy / h

♦ = 137Cs

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
EURISYS	3G10	MINIATURE	460		X			10		1		
EURISYS	4G15	MINIATURE	550		X			10				
EURISYS	4G60M	MINIATURE	500		X			10		1		
FORMER USSR	3043	PANCAKE	400	X	X	X				240		
FORMER USSR	BETA 1	PANCAKE	675			X				2700		
FORMER USSR	BETA 2	PANCAKE										
FORMER USSR	BETA 2-2	PANCAKE										
FORMER USSR	BETA 2M1	PANCAKE										
FORMER USSR	BETA-1	PANCAKE			X					120		7.0
FORMER USSR	BETA1-1	PANCAKE			X					120		7.0
FORMER USSR	BETA-2	PANCAKE			X					200		15.0
FORMER USSR	BETA2-2	PANCAKE			X					200		15.0
FORMER USSR	BETA2M	PANCAKE				X				200		
FORMER USSR	BETA2M1	PANCAKE				X				200		
FORMER USSR	CBM20-1	HOT DOG			X	X				800		
FORMER USSR	CI8B	PANCAKE			X					400		30.0
FORMER USSR	CI8B1	PANCAKE			X					400		30.0
FORMER USSR	SPA-8	scintillator	1000			X		12		300		
FORMER USSR	SBM-20 CBM	HOT DOG	400		X	X	10.2 + 07	190		780	22.0%	
Vacutronik	RAM 63-2	scintillator	1100		X	X	100 + 00	1				
Vacutronik	RAM 63-3	scintillator	1350	X			1.00 + 00	1				
F & H	FHZ 72	HOT DOG	450		X	X	2.25 + 01			1200		
F & H	FHZ 73	HOT DOG	450		X	X	2.25 + 01			1200		
F & H	FHZ 74	HOT DOG	450		X	X						
F & H	FHZ 76	HOT DOG	450		X	X						
F & H	FHZ 77A	END WINDOW	450	X	X	X						
G. & C.	XAI	END WINDOW	1480	X	X	X		50				
JOHNSON	GP200	END WINDOW	900	X	X	X		150		2500		9.1
JOHNSON	HP 265	scintillator	900	X	X	X		5		60000		14.0
JOHNSON	PPA-2T	PANCAKE	900	X	X	X				2500		14.0

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
LND	712	END WINDOW	500	X	X	X		90		1200		
LND	713	MINIATURE	575			X		28		420		
LND	714	MINIATURE	575			X		15		54		
LND	716	MINIATURE	550			X		11		19		
LND	719	THIN WALL	900		X	X		100		5275		
LND	720	THIN WALL	900		X	X		100		635		
LND	721	THIN WALL	900					95		2900		
LND	722	END WINDOW	900	X	X	X		150		2700		
LND	723	END WINDOW	900	X	X	X		200		1650		
LND	725	THIN WALL	900		X	X		150		1550		
LND	743	THIN WALL	900		X	X		100		3950		
LND	6306	HOT DOG	900		X	X						
LND	7224	END WINDOW	575	X	X	X		100		1700		
LND	7231	PANCAKE	900	X	X	X		90		1500		
LND	7232	END WINDOW	900	X	X	X		200		1650		
LND	7311	PANCAKE	900	X	X	X		50		3500		
LND	7802	THIN WALL	900					120		8150		
LND	72314	END WINDOW										
LND	72610	THIN WALL	900		X	X		20		175		
LND	73118	PANCAKE	900	X	X	X		90		3500		
LND	78017	THIN WALL	900		x	x		120		8150		

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
LUDLUM	133-2	ALOGEN	550			X		80		1000		15.0
LUDLUM	133-4	ALOGEN	550			X		80		100		15.0
LUDLUM	133-6	ALOGEN	550			X		50		30		15.0
LUDLUM	133-7	ALOGEN	460			X		50		4		15.0
LUDLUM	133-8	ALOGEN	460			X		50		1		25.0
LUDLUM	43-1	scintillator	1200	X					35.0%			83.0
LUDLUM	01/01/43	scintillator	1200	X	X				35.0%			83.0
LUDLUM	43-2	scintillator	1200	X					30.0%			15.0
LUDLUM	43-20			X	X							
LUDLUM	02/02/43	scintillator	1200	X	X							12.0
LUDLUM	43-40-2	scintillator										
LUDLUM	43-40-3											
LUDLUM	43-44	AIR PROPORTIONAL	2050	X								76.0
LUDLUM	43-44-1	AIR PROPORTIONAL	2050	X					8.0%			76.0
LUDLUM	43-5	scintillator	1200	X					13.0%			65.3
LUDLUM	43-65	scintillator	1200	X					17.0%			63.0
LUDLUM	43-68		900	X	X				15.0%			15.0
LUDLUM	43-89	scintillator	1200	X	X							100.0
LUDLUM	43-90	scintillator	1200	X								100.0
LUDLUM	43-92	scintillator	1200	X					20.0%			100.0
LUDLUM	43-93	scintillator	1200	X					20.0%			100.0
LUDLUM	44-1	scintillator	1200		X							11.6
LUDLUM	44-10	scintillator	1200		X					900		
LUDLUM	44-11	scintillator	1200		X					900		
LUDLUM	44-110	TRITIUM DET.	1700		X							126.0
LUDLUM	44-116	scintillator	1200		X							125.0
LUDLUM	44-142	scintillator	1200		X							100.0
LUDLUM	44-17	scintillator	1200			X				140		
LUDLUM	44-172											
LUDLUM	44-2	scintillator	900			X			13.0%	175		4.9
LUDLUM	44-20	scintillator	1200			X				2300		125.0
LUDLUM	44-21	scintillator				X	X					

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α	Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr ¹³⁷ Cs	Co60 γ	PROBE AREA cm ²
LUDLUM	44-25	PANCAKE	900	X	X	X					3300		
LUDLUM	44-26	PANCAKE	900	X	X	X					9900		
LUDLUM	44-3	scintillator	900			X					675		5.0
LUDLUM	44-38	COMPENSATE D			X	X							
LUDLUM	44-40	PANCAKE	900		X	X					3300		
LUDLUM	44-40-2	PANCAKE	900	X	X	X					3300		
LUDLUM	44-6	SIDEWALL	900		X	X		95			1200		15.5
LUDLUM	44-62	scintillator	1200			X					66		
LUDLUM	44-7	END WINDOW	900	X	X	X					2100		
LUDLUM	44-89	PANCAKE	900	X	X	X					12K		63.0
LUDLUM	44-9	PANCAKE	900	X	X	X	19.8-07	80		15.0%	3300		15.0
LUDLUM	09/18/44	PANCAKE	900	X	X	X	19.8 to 07	80		15.0%	3300		15.0
LUDLUM	44-92	XENON GAS			X	X							140.0
LUDLUM	44-94	PANCAKE	900	X	X	X					12K		
LUDLUM	44-98	scintillator			X								11.8

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
MILITARY	5979	END WINDOW	900	X	X	X		150		2700		
MILITARY	7616	END WINDOW	900	X	X	X		70		500		
MILITARY	8767	PANCAKE	900	X	X	X		50		3500		
MILITARY	JAN5979	END WINDOW	900	X	X	X		150		2700		
MILITARY	JAN7616	END WINDOW	900	X	X	X		70		500		
ROTEM	2147	PANCAKE	875	X	X	X				3500		
ROTEM	GM-10	PANCAKE	875	X	X	X	21 + 07			3500		10
ROTEM	GM-40	scintillator	875			X						
ROTEM	GM-41	scintillator	875			X						
ROTEM	GM-42	scintillator	875			X						
ROTEM	IC-10	IONIZZ.	875			X						
ROTEM	PA-100	IONIZZ.	875	X					26%			100.0
ROTEM	PM-10	scintillator	875			X						
ROTEM	PM-11	scintillator	875			X						

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr ^{137}Cs	Co60 γ	PROBE AREA cm ²
SAINT-GOB.	803	MINIATURE	575		X	X		28		475		
SAINT-GOB.	1504	MINIATURE	500			X		90		1400		
SAINT-GOB.	1504-1	MINIATURE	500			X		110		1400		
SAINT-GOB.	1611-PT	HIGH-SENS.	900			X		100		5000		
SAINT-GOB.	1620-PT	HIGH-SENS.	700			X		100		8500		
SAINT-GOB.	1625-PT	HIGH-SENS.	950			X		100		12850		
SAINT-GOB.	1915-PT	HIGH-SENS.	900			X		150		5800		
SAINT-GOB.	1916-PT	HIGH-SENS.	1000			X		150		6350		
SAINT-GOB.	3304-W	END WINDOW	575	X	X	X		175		1700		
SAINT-GOB.	50CM2		900	X	X	X		100		13400		
SAINT-GOB.	G1200	Cylindrical	500			X		90		1400		
SAINT-GOB.	G1210	Cylindrical	450			X		200		5200		
SAINT-GOB.	G1220	Cylindrical	450			X		210		9000		
SAINT-GOB.	G1221-2	HIGH-SENS.	450			X		210		9000		
SAINT-GOB.	G1300	MINIATURE	550		X	X		11		19		
SAINT-GOB.	G1301	MINIATURE	550			X		13		16		
SAINT-GOB.	G1310	MINIATURE	575		X	X		15		85		
SAINT-GOB.	G1313	MINIATURE	575			X		15		85		
SAINT-GOB.	G1321	MINIATURE	575			X		55		475		
SAINT-GOB.	G1421	END WINDOW	575	X	X	X		230		2300		
SAINT-GOB.	G1452		500	X	X	X		100		1700		
SAINT-GOB.	N1004		500	X	X	X		60		1500		
SAINT-GOB.	N1005	END WINDOW	900	X	X	X		100		3350		
SAINT-GOB.	N1008		900	X	X	X		100		3350		
SAINT-GOB.	N106-3P	Cylindrical	900		X	X		100		2200		
SAINT-GOB.	N107-3P	Cylindrical	900		X	X		100		5200		
SAINT-GOB.	N108-3P	Cylindrical	900		X	X		100		3300		
SAINT-GOB.	N112	Cylindrical	900		X	X		150		1500		
SAINT-GOB.	N112HS	Cylindrical	900		X	X		150		2000		
SAINT-GOB.	N112X	Cylindrical	900		X	X		150		1100		
SAINT-GOB.	N114	Cylindrical	900		X	X		100		800		
SAINT-GOB.	N302	MINIATURE	900			X		20		125		
SAINT-GOB.	N309-3P	Cylindrical	900			X		100		2200		
SAINT-GOB.	N310-3P	Cylindrical	900			X		100		4700		

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT uS	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
SAINT-GOB.	N358-9,1	HIGH-SENS.	950			X		100		12850		
SAINT-GOB.	N3785		450		X	X		200		8500		
SAINT-GOB.	N378S	HIGH-SENS.	450			X		200		9000		
SAINT-GOB.	NP334-6	HIGH-SENS.	900			X		150		5800		
SAINT-GOB.	NP334-6,6	HIGH-SENS.	1000			X		150		6350		
SAINT-GOB.	NP334-8	HIGH-SENS.	900			X		100		8500		
SAINT-GOB.	NP358-1,8	HIGH-SENS.	700			X		100		2600		
SAINT-GOB.	NP358-6	HIGH-SENS.	700			X		100		5500		
SAINT-GOB.	NP358-8	HIGH-SENS.	700			X		100		8500		

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
TGM	5368		450			X						
TGM	mc71		450			X						
TGM	N1002	PANCAKE	900	X	X	X		50		3500		
TGM	N1002-1	PANCAKE	900	X	X	X		50				
TGM	N1004	PANCAKE	900					90		1500		
TGM	N1006	PANCAKE	900					70		500		
TGM	N106	THIN WALL	900					75		2900		
TGM	N107	THIN WALL	900					100		5275		
TGM	N112	THIN WALL	900					150		1550		
TGM	N114	THIN WALL	900					90		635		
TGM	N115-1	THIN WALL	550					11		19		
TGM	N116-1	THIN WALL	575					15		54		
TGM	N117-1	THIN WALL	575					28		420		
TGM	N119	THIN WALL	900					150		4800		
TGM	N201	END WINDOW	900					150		2700		
TGM	N202	END WINDOW	750					50		50		
TGM	N204	END WINDOW	900									
TGM	N204 / MHV	END WINDOW										
TGM	N205	END WINDOW	500					90		1200		
TGM	N206	END WINDOW	575					100		1700		
TGM	N210	END WINDOW	900					200		1650		
TGM	N210 / BNC	END WINDOW	900					200		1650		
TGM	N305	THIN WALL	500					90		1200		
TGM	N309	THIN WALL	900					100		1880		
TGM	N310	THIN WALL	900					100		3950		
TGM	N320	THIN WALL	900					100		950		

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α	Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²
THERMO	44-88	END WINDOW	900	X	X	X					3300		
THERMO	A50L	scintillator			X								0.6
THERMO	AC 3-7	scintillator	1000	X				6					0.5
THERMO	AC 3-8	scintillator	1000	X				6					0.5
THERMO	AP2 / 4A	scintillator			X								0.5
THERMO	AP4 / 4A	scintillator			X								0.2
THERMO	AP5AD	scintillator			X								0.5
THERMO	AP5RA	scintillator			X								1.0
THERMO	AP6A	scintillator			X								6.0
THERMO	BP19AD	scintillator				X					3000		100.0
THERMO	BP7 / 4C	scintillator				X					1500		1.4
THERMO	BP1 / 4A	scintillator				X					1800		1.4
THERMO	BP13A	scintillator				X							80.0
THERMO	BP17A	scintillator				X							600.0
THERMO	BP19DD	scintillator				X					3000		100.0
THERMO	BP4 / 4A	scintillator				X					1500		20.0
THERMO	BP4 / 4C	scintillator				X					1500		20.0
THERMO	BP7 / 4A	scintillator				X							80.0
THERMO	DP2 / 4A	scintillator				X							600.0
THERMO	DP2R / 4A	scintillator				X	X						50.0
THERMO	DP6AD	scintillator				X	X						100.0
THERMO	DP8A	scintillator				X	X						600.0
THERMO	GP20B / R	END WINDOW	450				X						
THERMO	GP21B / R	END WINDOW	500				X						
THERMO	HP 100 CGS	GAS P10	1800	X	X								
THERMO	HP 190-01	END WINDOW	900	X	X	X		200		6.0%	3	10.0%	
THERMO	HP 190A	END WINDOW	900	X	X	X	1 + 00	200			2500		
THERMO	HP 210	PANCAKE	900	X	X	X	1 + 00	80		25.0%	3600	16.0%	15.5
THERMO	HP 220A	PANCAKE	600	X	X	X							
THERMO	HP 260												
THERMO	HP 270	PANCAKE	900	X	X	7.2 + 07	112				1200		
THERMO	HP 280												
THERMO	HP 290	PANCAKE	550	X	X	7.2 + 07	120				1200		
THERMO	HP 300	GM											

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm2
THERMO	HP 360	PANCAKE	900	X	X	X	21.6 + 07	50		3600	16.0%	15.5
THERMO	HP 380 AB	PANCAKE	900		X	X				1200		
THERMO	HP 380A	PANCAKE	600	X					21.0%			100.0
THERMO	HP 380B		900		X					1200		
THERMO	HP 100CGS	GAS P10			X	X	X					
THERMO	HP 220							100			19	
THERMO	HP 220A		600			X	1.55 + 06	60				1.0
THERMO	HP 230A		900		X	X						
THERMO	HP 260	PANCAKE	500		X	X		80		3600		
THERMO	HP 280											
THERMO	HP 330	PANCAKE	1550	X	X	X						
THERMO	HP 340											
THERMO	HP 350											
THERMO	HP 370	PANCAKE	1750	X	X	X						
THERMO	IGP24A / SV		550							137		
THERMO	LEG-1	scintillator	1000			X	100 + 00	12			60	
THERMO	NRD	PROPORZ	1850			X	300 + 06	10				
THERMO	PG-2		1000			X				60K		
THERMO	PGM / ECPCM	PANCAKE	900					50		3600		15.5
THERMO	RCM-1		1200				2.80 to 01	13				
THERMO	RD-14			X	X							
THERMO	SAC-R5		800									
THERMO	SPA-1A		650	X			3.10 to 01	10				
THERMO	SPA-3	scintillator	1000			X		14		1200K		
THERMO	SPA-6	scintillator	1000			X		14		600K		
THERMO	SPA-9	scintillator	1000			X		12		400K		
THERMO	SW / GM		900					100		1600		
THERMO	WAM-4		1000			X	1.76 to 01	13				

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr 137Cs	Co60 γ	PROBE AREA cm ²	R	pF
VALVE	18500	AR	1050			x		75						
VALVE	18501	AR	1050			x		75						2.0
VALVE	18502		350		x	x		150						2.0
VALVE	18503	Ne Ar ALO	450			x		100					10M	2.0
VALVE	18504	Ne Ar ALO	450	x	x	x		100				63.5	10M	2.0
VALVE	18505	Ne Ar ALO	450	x	x	x		125				3.0	10M	2.0
VALVE	18506	Ne Ar ALO	475	x	x	x		225				6.0	10M	3.5
VALVE	18509-02	Ne Ar ALO	550		x	x		30					2M	1.0
VALVE	18509	Ne Ar ALO	550		x	x		60					10M	1.0
VALVE	18510	Ne Ar ALO	450		x			125					5M	4.0
VALVE	18511	XE	1500			x								2.0
VALVE	18513	rare gases	575	x	x			60				31.7		1.5
VALVE	18514	rare gases	600	x	x			250				605.0		1.5
VALVE	18515	Ne Ar ALO	575		x			150				3.1	10M	1.5
VALVE	18516	Ne Ar ALO	575		x			40				6.1	5M	1.3
VALVE	18517	ALO	1000					1					10M	5.5
VALVE	18518	ALO	1000					1					10M	8.0
VALVE	18519	Ne Ar ALO	450			x		35					4.7m	2.2
VALVE	18520	Ne Ar ALO	375			x		60					4.7m	4.5
VALVE	18523	Ne Ar ALO	600			x		70				455.0	4.7m	3.0
VALVE	18524-01	Ne Ar ALO	400		x	x		100				10.0	4.7m	2.5
VALVE	18526	Ne Ar ALO	450	x	x	x		200				6.1	10M	3.5
VALVE	18529	Ne Ar ALO	400			x							2M	0.5
VALVE	18533	Ne Ar ALO	400		x	x		100					4.7m	2.5
VALVE	18536	Ne Ar ALO	500	x	x	x		40				6.1	5M	1.3
VALVE	18537	Ar ALO	1000			x		150				3.1	4.7m	2.7
VALVE	18538	Kr ALO	1000			x		400				3.1	4.7m	2.7
VALVE	18545	Ne Ar ALO	500			x		200					4.7m	10.0
VALVE	18546	Ne Ar ALO	900		x			45					4.7m	5.0
VALVE	18550	Ne Ar ALO	500		x	x		50					5M	1.1
VALVE	18552	Ne Ar ALO	600		x	x		70					2M	4.0

see website <http://www.vacutech-gmbh.de> > Product> Geiger-Müller-Zählrohr Typenauswahl

TYPE	Sensitivity			Dose-Rate-Range ($\mu\text{Sv/h}$ / $\mu\text{Gy/h}$) ²⁾	Counting Rate [^{137}Cs] at 1 $\mu\text{Gy/h}$ (counts/s)	Dead-time (μs)	Background shielded ³⁾ (counts/min)	Plateau					
	Band		max.Length (mm)					Range (V)	Slope (%/100V)				
	α	β											
70 003	-	-	43	1 ... 10^5	2.2	≤ 120	≤ 20	400 ... 600	8				
70 003 A/E ¹⁾	-	-	45	1 ... 10^5	2.6	≤ 120	≤ 8	400 ... 600	8				
70 013	-	-	170	0.3 ... 10^4	10	≤ 100	≤ 60	400 ... 600	10				
70 013 A/E ¹⁾	-	-	167	0.3 ... 10^4	7.5	≤ 100	≤ 60	400 ... 600	10				
70 015	-	-	35	10^2 ... 10^7	0.04	≤ 13	≤ 1	500 ... 600	30				
70 015 A/E ¹⁾	-	-	35	10^2 ... 10^7	0.04	≤ 13	≤ 1	500 ... 600	30				
70 016	-	-	37	10 ... 4×10^6	0.16	≤ 15	≤ 2	500 ... 650	15				
70 016 A/E ¹⁾	-	-	35	10 ... 4×10^6	0.16	≤ 15	≤ 2	500 ... 650	15				
70 017	-	-	57	2 ... 3×10^5	0.73	≤ 25	≤ 5	400 ... 550	10				
70 017 A/E ¹⁾	-	-	59	2 ... 3×10^5	0.72	≤ 25	≤ 5	400 ... 550	10				
70 018	-	-	43	10^2 ... 2×10^7	0.02	≤ 20	≤ 2	520 ... 620	30				
70 018 A/E ¹⁾	-	-	55	10^2 ... 2×10^7	0.02	≤ 20	≤ 2	520 ... 620	30				
70 019	-	-	49	1 ... 5×10^4	2.1	≤ 60	≤ 7	400 ... 600	4				
70 019 A/E ¹⁾	-	-	51	1 ... 5×10^4	1.7	≤ 60	≤ 7	400 ... 600	4				
70 030	-	-	45	1 ... 10^5	2.5	≤ 65	≤ 20	400 ... 600	8				
70 030 A/E ¹⁾	-	-	45	1 ... 10^5	1.5	≤ 65	≤ 8	400 ... 600	8				
70 031	-	-	300	0.2 ... 3×10^3	16	≤ 150	≤ 120	400 ... 600	10				
70 031 A/E ¹⁾	-	-	300	0.2 ... 3×10^3	18	≤ 150	≤ 100	400 ... 600	10				
70 035	-	-	109	0.3 ... 3×10^4	5.5	≤ 100	≤ 50	400 ... 550	8				
End-window	Energy Range			Window			Dead-time (μs)	Background shielded ³⁾ (counts/min)	Plateau				
	α	β	X	\varnothing (mm)	Thickness (mg/cm ²)	Material			Range (V)	Slope (%/100V)			
	(MeV)	(keV)	(keV)										
70 071	3.5	50	3	18	1.5 ... 2	Mica	≤ 120	5	420 ... 650	5			
70 072	3.5	50	3	13	1.5 ... 2	Mica	≤ 90	7	400 ... 600	4			
70 074	3.5	50	3	36	1.5 ... 2	Mica	≤ 120	24	420 ... 650	3			
70 075	3.5	50	3	45	1.5 ... 2	Mica	≤ 30	24	850 ... 1050	10			

¹⁾ with compensation filter: A=Ambient Dose Equivalent (H*10), E=Air Kerma/Exposure

²⁾ A in [$\mu\text{Sv/h}$], E in [$\mu\text{Gy/h}$] ; for the uncompensated types the range is given in dose rate unit at 662 keV [^{137}Cs]

³⁾ shielded with 5cmPb+0.2cm Al

PRODUCER	MODEL	PROBE	OPERATING VOLTAGE HV	α	β	γ	CC	DT us	α Pu 239 - 4P	$\beta + \gamma$ cpm / mR / hr ^{137}Cs	Co60 γ	PROBE AREA cm ²
VICTOREN	301	HOT DOG	900		X	X		100		720		
VICTOREN	OCD-101	HOT DOG	900		X	X		100		720		
VICTOREN	OCDD-103	HOT DOG	900		X	X		100		720		

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

see website www.lndinc.com > Product > Cross Reference Chart to Other Mfg. Products

LND Type	Phillips Amperex	TGM Detectors	Centronics	Mullard	LND Type	Phillips Amperex	TGM Detectors	Centronics	Mullard
72314	18526	N / A	ZP1430	MX169	7103	N / A	NP322-2	N / A	N / A
72327	18506	N / A	ZP1431	MX149	720	N / A	N114	N / A	N / A
7311	N / A	N1002 / 8767	N / A	N / A	7242	18515	N / A	ZP1441	MX152
73118	18546	N1006	ZP1460	MX167	72412	N / A	N / A	ZP1442	N / A
743	N / A	N310 / 3P	N / A	N / A	712	N / A	N / A	ZP1401	N / A
719	N / A	N107 / 3P	ZP1860	N / A	7121	18503	N / A	ZP1200	MX146
72514	N / A	N / A	B12N	N / A	7124	18504	N205	ZP1400	MX147
78016	18520	N / A	ZP1210	MX120	7128	N / A	N / A	ZP1201	N / A
7807	N / A	N / A	ZP1221	N / A	72310	N / A	N1003	N / A	N / A
78017	18545	N / A	ZP1220	MX145	725	N / A	N112	N / A	N / A
72511	N / A	N / A	B12C	N / A	7231	18536	N / A	ZP1490	MX166
71322	N / A	N117-1S / C1321	ZP1321	N / A	72315	18516	N / A	ZP1452	N / A
7256	N / A	NP334-6	N / A	N / A	72216	N / A	N / A	ZP1470	MX123
716	18529	N115-1 / C1300	ZP1300	MX163	7224	18505	N / A	ZP1410	MX148
7165	N / A	N115-1S1 / C1301	ZP1301	N / A	723	N / A	N210-1	N / A	N / A
7437	N / A	NP358-9.1	N / A	N / A	7232	N / A	N210 / BNC	N / A	N / A
714	18509	N116-1 / C1310	ZP1310	MX151	721	N / A	N106 / 3P	ZP1850	N / A
45697	18511	N / A	ZP1610	MX161	72118	18555	N / A	ZP1330	MX177
7149	N / A	N / A	ZP1313	N / A	72219	18507	N / A	ZP1600	MX159
71412	N / A	N116-1SE / C1312	ZP1311	MX189	72231	N / A	N201	N / A	N / A
72611	N / A	N302	N / A	N / A	72233	N / A	N / A	ZP1481	MX168
78034	N / A	N378 / BNC	N / A	N / A	740501	N / A	NP315-4	ZP1810	N / A
713	18550	N117-1 / C1320	ZP1320	MX164	7436	N / A	NP358-5.75 / 3P	N / A	N / A
7133	N / A	N / A	M6H	N / A					
7139	N / A	N / A	ZP1324	N / A					
7102	N / A	N222	N / A	N / A					

see website <http://www.canberra.com/products/438339.asp>

	CANBERRA	Centronics	LND	Saint Gobain
Min. Detectors	T2411	ZP1310	714	N116-1 / C1310

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

see website <http://www.vacutec-gmbh.de> > Product> Geiger-Müller-Zählrohr Cross-Referenzliste

VacuTec	Centronics	Philips Amperex	LND	Mullard	TGM Detectors
70003	ZP1200	18503	7121	MX146	
70 003 E	ZP1201		71210		
70 003 A	ZP1202				
70013	ZP1210	18520	78016	MX120	
70 013 E					
70 013 A					
70015	ZP1300	18529	716	MX163	N115-1 / C1300
70 015 E	ZP1301		7165		N115-1S1 / C1301
70 015 A	ZP1304				
70016	ZP1310	18509	714	MX151	N116-1 / C1310
70 016 E	ZP1313		7149		
70 016 A	ZP1314				
70017	ZP1320	18550	713	MX164	N117-1 / C1320
70 017 E	ZP1321		71322		N117-1S / C1321
70 017 A	ZP1324		7139		
70019	ZP1200	18503	7121	MX146	
70 019 E	ZP1201		71210		
70 019 A	ZP1202				
70031	ZP1220	18545	78017	MX145	
70 031 E	ZP1221		7807		
70 031 A	ZP1221 / 02				
70071			7241		
70072	ZP1400	18504	7124	MX147	
70074	ZP1430	18526	72314	MX169	
70075	ZP1460	18546	7312	MX167	

PROBE SELECTION GUIDE by Massimiliano De Luigi - iz4kjs@tiscali.it AND salvatoregiarratana-labx@yahoo.it

See website http://www.centronic.co.uk/geiger_muller_tubes_cross_reference.htm

ZP	185	MX	US
ZP1200	18503	MX146	
ZP1210	18520	MX120 / 01	
ZP1220	18545	MX145	
* ZP1230		MX180	
* ZP1240		MX119	
ZP1300	18529	MX163	
ZP1310	18509	MX151	
* ZP1311		MX189	
* ZP1311		ZP1100	
ZP1320	18550	MX164	
ZP1330	18555	MX177	
ZP1400	18504	MX147	
ZP1410	18505	MX148	
ZP1430	18526	MX169	
ZP1431	18506	MX149	
ZP1441	18515	MX152	
ZP1451	18536	MX166	
* ZP1460	18546/01	MX167 / 01	
ZP1470		MX123	
ZP1480		MX168 / 02	
ZP1481		MX168	
* ZP1500		ZP1083	
* ZP1501		ZP1080	
* ZP1520	18525	MX124-01	
* ZP1530		MX142	
* ZP1550		MX188	
ZP1600	18507	MX159	
ZP1610	18511	MX161	
ZP1700	18518	MX155	
ZP1800			171g
* ZP1810			181G2
* ZP1820			78L
* ZP1830			79L
* ZP1840			560n
* ZP1850			90NB3
* ZP1860			912NB3

A collection (non-exhaustive) of sites WEB

Various info in Italian

<http://digilander.libero.it/dadano1/Fisica.htm>
http://spazioinwind.libero.it/andrea_bosi/appunti.htm
<http://www.webalice.it/carlo.scorsone/>
<http://barsanti.tripod.com/index.html>
<http://www.chirio.com/index.htm>
<http://www.archivionucleare.com/index.php/page/1/>
<http://web.tiscalinet.it/vcoletti/educational/materia/index.html>
<http://digilander.libero.it/ilnucleare/>
<http://www.lnf.infn.it/lnfadmin/radiation/educational.html> <http://www.newscientist.com/topic/nuclear>
<http://nuovonucleare.splinder.com/>

Tools and more

<http://www.vacutech-gmbh.de/>
<http://www.lndinc.com/>
<http://www.centronic.co.uk/index.htm>
<http://www.canberra.com/>
<http://www.detectors.saint-gobain.com/Default.aspx>
<http://www.ludlums.com/>
<http://www.eberlineservices.com/index.htm>
<http://www.thermoscientific.com/wps/portal/ts/HOME>
<http://www.hilger-crystals.co.uk/prior/stand.htm>
<http://www.rotemi.co.il/>
<http://www.ortec-online.com/Solutions/RadiationDetectors/index.aspx>
<http://seintl.com/>
<http://www.bubbletech.ca/>
<http://polimaster.us/>
<http://www.radcal.com/>
<http://www.eljentechnology.com/>
http://www.apantec.com/product_services.asp
<http://www.geigercounters.com/>
<http://www.radshelters4u.com/>
http://www.beejewel.com.au/research/Bee_Research/home.html
<http://www.tubedata.info/>
<http://tubedata.itchurch.org/index.html>

Various info in other languages

<http://carlwillis.wordpress.com/>
<http://www.vaughns-1-pagers.com/science/radiation-detection.htm>
<http://www.chetan.homepage.t-online.de/sonstig/ram63.htm>
<http://sites.google.com/site/anilandro/Home>
<http://www.dangerouslaboratories.org/>
<http://sites.google.com/site/sciradioactive/>
<http://home.comcast.net/~prutchi/>
<http://hyperphysics.phy-astr.gsu.edu/hbase/hframe.html>

Museums and historical archives

<http://www.museumofquackery.com/welcome.htm>
<http://national-radiation-instrument-catalog.com/>
<http://www.orau.org/ptp/museumdirectory.htm>
<http://www.civildefensemuseum.com/>

Sources and related

<http://www.spectrumtechniques.com/>
<http://www.unitednuclear.com/>
<http://www.imagesco.com/geiger/radioactive-sources.html>
<http://www.anythingradioactive.com/>

Software

<http://www.qsl.net/dl4yhf/spectra1.html>
http://seintl.com/products/observer_software.html
<http://www.physics.usyd.edu.au/~marek/>
<http://www.blackcatsystems.com/index.html>
<http://sourceforge.net/projects/cdvcounter/>
<http://www.anythingradioactive.com/CDVCounter/help.html>
<http://www.radprocalculator.com/Index.aspx>
<http://ea4eo.zure.es/ugp.html>

satisfied users

<http://radgoes.blogspot.com/>

Thermo Radiometrie

1949	Founded by Mr. Fieseke and Mr. Hoepfner as Frieske & Hoepfner GmbH, a company specialized in precision machinery, hydraulic equipment tools, radiation monitoring and industrial gauging technology.
1954	Acquired by the owner of FAG Kugelfischer, Although the company still operated under the name of Frieske und Hoepfner GmbH, continuing to manufacture practically the same product range.
1981	Integrated as three product divisions, Hydraulic & Control, Radiation Monitoring and Radiometrie into FAG Kugelfischer at cooperaton with 38,000 employees.
1986	In March the Radiometrie division acquired Daystorm (Gloucester, England) and Nucleometre (Sarcelles, France) from Schlumberger and gauging formed the largest company in Europe.
1993	Thermo Instrument Systems acquired Radiometrie as of Nov. 1, 1993. In 1994 Eberline Instrument GmbH was formed.
1996	Thermo Instrument Systems spun out its divisions Eberline Radiometrie and Gamma Metrics to form Metrika Systems Corporation.
1998	Metrika Systems Corporation acquired the gauging metals division of Honeywell-Measurex, forming Radiometrie, the world's largest gauging company with three plants in Germany, UK and USA.



http://www.ludlums.com/images/stories/news_letters/Don%20Ludlum%20Story.pdf



<http://www.centronic.co.uk/history.htm>

Founded in 1945 by Gilbert Tomes and Alec Tidmarsh, Centronic, or 20th Century Electronics as it was then known, started life in the back bedroom of Gilbert Tomes' house in Kent, England.

His work on electron tubes Within the television industry and his interest in radiation detection led to the creation of 20th Century Electronics for the commercial development and manufacture of cathode ray tubes and Geiger-Müller. He Became only owner of the firm in 1949 When It Became a limited company, 20th Century Electronics Limited. By concentrating on chosen specialties of radiation detection and optical sensing, the company grew rapidly to become a world leader in its area of expertise, with many cutting edge innovations Arising on the way. With over 50 years experience in meeting the challenge of change, the firm continues to be as much as ever to "hive of activity".



Saint-Gobain Crystals is an operating unit of Compagnie de Saint-Gobain, Which is based in Paris, France.

Saint-Gobain was created in 1665 by Louis XIV's Minister of Finance, Jean-Baptiste Colbert, to break Venice's monopoly over the glass trade. Saint-Gobain supplied the mirrors for the Hall of Mirrors in the Palace of Versailles in 1684.

It has been established since 1853 in Germany, in 1889 in Italy, 1904 in Spain and Benelux, in 1937 in Brazil, in 1967 in the United States.

The Foundation of Saint-Gobain Crystals, Scintillation Products

1930's	Harshaw Chemical Company is the first major manufacturer to develop and produce scintillation crystals.
1940's	Quartz & Silica, a subsidiary of Saint-Gobain, begins production of optical crystals and scintillation crystals.
1969	Bicron Corporation is established and begins production of NaI (Tl) scintillation ingots.
1990	Saint-Gobain acquires Bicron Corporation and Harshaw brand products from Engelhard.
1992	Crismatec-Grenoble is acquired. Crismatec Becomes the new name for the Quartz & Silica entity.
1997	Bicron Products Private Limited (BPPL) production facility is opened in Bangalore, Karnataka, India
1999	Bicron TGM acquires Detectors and Gamma Laboratories.
2000	All of the above businesses and brand names are united under the name Saint-Gobain.
2002	Bicron Radiation Measurement and Protection division is sold to Thermo Electron.
2003	Introduction trademarks of new scintillation crystals Lanthanum Chloride, Lanthanum Bromide and LYSO, Which are later, marketed under the brilliance and Prelude
2008	Saint-Gobain Crystals Scintillation headquarters and manufacturing operations move to new facility in Hiram, Ohio.
	http://www.detectors.saint-gobain.com/History.aspx